

An Approach to Improve the Misalignment and Wireless Power Transfer into Biomedical Implants Using Meandered Wearable Loop Antenna

Muayad Kod¹, Jiafeng Zhou^{2*}, Member, IEEE, Yi Huang², Senior Member, IEEE, Muaad Hussein², Abed P. Sohrab², and Chaoyun Song²

¹Electrical and Electronics Engineering, University of Kerbala, Kerbala, Iraq

²Electrical Engineering and Electronics, The University of Liverpool, Liverpool, U.K.

* Jiafeng.Zhou@liv.ac.uk

Abstract: An approach to improve wireless power transfer (WPT) to implantable medical devices using loop antennas is presented. The antenna exhibits strong magnetic field and dense flux lines distribution along two orthogonal axes by inseting the port inside the antenna area. This design shows excellent performance against misalignment in the y-direction and higher WPT as compared with a traditional square loop antenna. Two antennas were optimized based on this approach, one wearable and the other implantable. Both antennas work at both the ISM (Industrial, Scientific and Medical) band of 433 MHz for WPT and the MedRadio (Medical Device Radiocommunications Service) band of 401-406 MHz for communications. To test the WPT for implantable medical devices, a miniaturized rectifier with a size of 10 mm × 5 mm was designed to integrate with the antenna to form an implantable rectenna. The power delivered to a load of 4.7 kΩ can be up to 1150 μW when 230 mW power is transmitted which is still under the safety limit. This design can be used to directly power a pacemaker, a nerve stimulation device or a glucose measurement system which requires 70 μW, 100 μW and 48 μW DC power respectively.

1. Introduction

Wireless power transfer (WPT) to implantable devices has attracted significant attention in last decade. It is a promising choice for delivering power to the implants which may avoid the surgery required to replace batteries [1]. This power transfer takes place when a voltage is induced at a receiver due to electric and magnetic fields generated by an external transmitter [2].

Traditionally two major techniques of delivering power wirelessly into the implant exist. The first one is far-field transmission using antennas [3] - [9]. An external antenna is placed away from the body to power and communicate with implants through an implantable antenna. This approach restricts the patient's mobility and exposes the whole body to the radiated power. The second technique is the inductive coupling between two coils [10] - [19]. These coils should be kept aligned well otherwise the strong electromagnetic coupling will be lost.

Inductive coupling is not restricted to coils. Antennas can be used in power transmission based on this technique if it is placed in close proximity within the near field region. These antennas are wearable on the body and used to wirelessly charge as well as communicate with implants. Loop antennas are widely used for this purpose in the literature because of the high magnetic field in the near field region. A pair of square loop antennas was used to characterize the effect of human head on the transmission of RF signal at the MedRadio band in [20]. Another pair of circular loop and triangle patch antennas were used to improve communications with implants in [21]. In [22] a near field wireless power link was established between a brain implantable bowtie antenna and an off body exterior loop antenna. A metasurface-based WPT link consists of

transmitting patch and receiving implantable loop antenna is proposed in [23]. A dual broadband loop antenna was developed for WPT and communications with implantable antennas in [24]. A pair of square loop antennas was used for WPT in [25]. A parasitic patch implantable antenna was utilized to improve the WPT with a transmitting array antenna [26]. A multiband antenna with T-shaped ground slot is proposed for WPT and Telemetry [27]. A circular loop antenna and an implantable cubic loop antenna were used for powering Brain Machine Interfacing in [28]. In these applications, it is very difficult to know the location and orientation of the implants accurately. Consequently, the misalignment issue is expected to occur.

Misalignment is one of the most challenging issues for WPT. Previous works have been conducted to investigate and resolve this issue. Multiple circular coils were used as a solution for retinal implant system to improve WPT and reduce the misalignment effect in [29]. Typical receiver orientation and position for better WPT based on the magnetic field distribution were studied using spiral coils to tolerate the misalignment in [15]. In [30], a repeater coil between multiple transmitting and receiving coils was used to reduce the misalignment effect and improve WPT by altering the orientation of the repeater. In [31], an adaptive impedance matching at the transmission side was used to improve axial misalignment. Other researchers suggested a solution to solve the misalignment by using parallel and orthogonal winding at the secondary coil in [32] and [33]. In [34] a mix of circular spiral and helical coils in bowl shape as a transmitter and rectangular spiral and helical coils with ferrite core as a receiver have been used to compensate the misalignment issue. Another solution using square loop antennas was introduced in [35] by using distributed array of transmitting loops to improve lateral misalignment of WPT. Most of the

suggested solutions are complicated and bulky especially for biomedical applications. In this paper, a compact solution using loop antennas is introduced. This solution is planar and small in size. No matching solutions or extra array elements are required to improve the efficiency of WPT and the misalignment issue. Furthermore, this design can work on two bands MedRadio (401-406 MHz) and ISM (433 MHz). These make the proposed design very suitable for biomedical applications.

The paper is organized as follows: in Section II, the antenna design and performance analysis are presented. Section III focuses on the misalignment analysis between the wearable and implantable antennas. Section IV discusses the WPT measurement. Conclusions are finally given in Section V.

2. Antenna Design and Performance Analysis

Loop antennas are the most commonly used antenna types on the body because of the high magnetic field in the near field region. Magnetic field has negligible interaction with biological materials [2] and then the antenna is more robust against the detuning by the high permittivity of the body.

A loop antenna can be considered as a coil with one turn. The inductive coupling between two loops can be presented in the simplified circuit model as shown in Fig. 1, where L , R and C are the self-inductance, resistance and capacitance of an antenna respectively. The mutual coupling between two loops is denoted by M . The subscripts p and s refer to the primary and the secondary loops respectively.

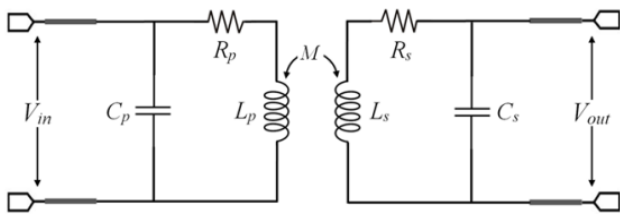


Fig. 1. Equivalent circuit of two coupled loops

The improvement of WPT comes from better coupling coefficient k due to higher M according to:

$$k = \frac{M}{\sqrt{L_p L_s}} \quad (1)$$

The traditional approach to improve WPT is to increase the magnetic field by increasing the self-inductance through adding more turns to the coil or increasing the length of the antenna conductor. This leads to higher induced voltage at the receiver according to Faraday law in equation (2) [2].

$$V_2 = i\omega\mu_0 \int H_1 \cdot ds \quad (2)$$

where V_2 is the induced voltage at a receiver, ω is the operating frequency, μ_0 is the permeability of free space, H is the magnetic field generated by a source at a receiver of

area S . However, any misalignment can cause the loss of the flux linkage and then the reduction in WPT.

WPT for implants is established between asymmetrical antennas because the secondary implantable antenna is much smaller than the primary wearable transmitter due to the high permittivity of body tissues. An accurate position for the secondary antenna with respect to the primary one is unguaranteed during implantation and hence the misalignment and then a reduction in WPT efficiency can occur.

It is important to find a proper design that can provide better coupling when the receiver encounters a misaligned position. An understanding of the flux lines distribution can help in modifying this distribution to get larger flux linkage with the receiver and then a higher coupling coefficient k .

A meandered loop antenna is proposed in this paper as shown in Fig. 2. The loop antenna with a perimeter of about one λ (wavelength) long behaves as a folded dipole antenna with two $\lambda/2$ dipoles. The directions of the currents along the two halves are the same as shown in Fig. 3(a). The surface current along each half will be maximal at the center and becomes weaker at the ends. These currents generate a magnetic field around the conductor in a direction following the right hand rule. As a result, the generated fields will be in opposite directions in the center area of the conventional loop antenna and will cancel out each other. This leads to weak magnetic field at the middle area and stronger at edges as will be seen in sections II and III.

The magnetic field is distributed in closed lines around the source conductor. Larger induced voltage can be generated at the receiver when these lines cut the effective parts of the receiver antenna in an appropriate direction. This means that the z components of magnetic lines from horizontal conductor along x -axis shown in Fig. 3(c) are distributed in vertical closed lines. It can induce voltage at the horizontal conductor of the receiver while it is less effective at the vertical conductors. The same scenario is true for the horizontal closed lines fields from vertical conductor. A reshape for the generated magnetic field distribution at the target receiver is important to design efficient WPT system.

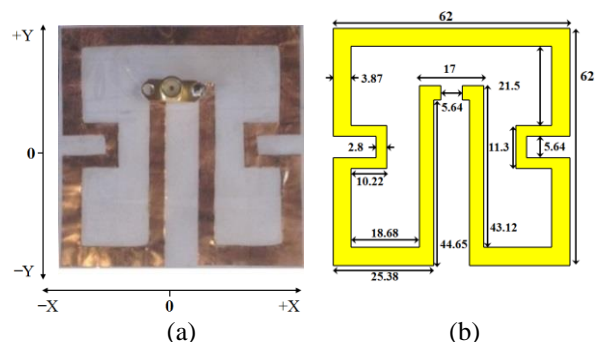


Fig. 2. The proposed antenna: (a) Fabricated prototype (b) detailed dimensions in mm.

A. Configuration of the Wearable Meandered Loop Antenna

Meandered loop antenna is a technique that helps in reducing the antenna size [36]. The magnetic field in the internal area of the loop can be consolidated through meandering the antenna in a specific way to create a

constructive combination. A redirection of the surface current is proposed in this work as shown in Fig. 3(b). A strong magnetic field and redistribution to the magnetic flux can be generated in almost the whole area of the antenna. This is can achieved by dragging the exciting port into the internal area. The antenna has been meandered more at the sides to get a smaller antenna size at the same operating frequency. The new design has achieved two advantages: the first one is to generate combined magnetic fields constructively in most of the antenna area. The second is that the generated magnetic field is strong along two different axes in the xy-plane of the antenna. Currents along two axes generate magnetic lines distribution vertically and horizontally in closed lines and the generated field is strong in almost all antenna area as shown in Fig. 3(c). The dense orthogonal lines provide better coupling with the receiver at different locations and then improve WPT. Furthermore, it will improve the misalignment issues as will be discussed in section III.

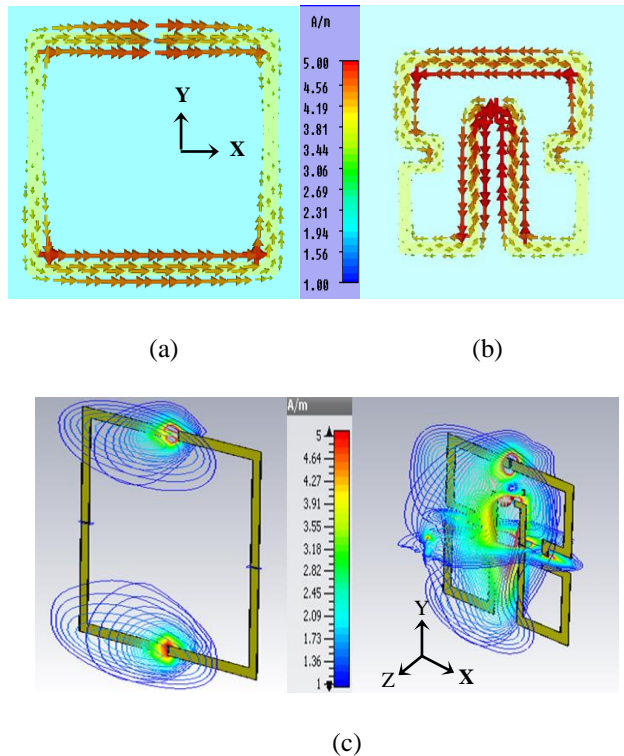


Fig. 3. (a) Surface current distribution in a square loop antenna. (b) Surface current distribution in the proposed meandered loop antenna. (c) Magnetic field distribution for both antennas.

The proposed antenna covers both the MedRadio band and the ISM band of 433 MHz. This antenna is fabricated by cutting a copper sheet into shape. The thickness of the copper sheet is 0.1 mm. This thickness does not significantly affect the performance of the antenna. The simulated radiation efficiency and gain of this antenna on a body model that consists of 4 layers as shown in Fig. 4 are 1.13% and -16.5 dB respectively. The properties of these layers are defined as a bio tissue from CST Voxel family with broadband properties from 0.1 – 3 GHz as shown in Table I. The thicknesses of these layers are 2 mm, 1 mm, 2 mm and 95 mm for clothes, skin, fat and muscle, respectively. These values are expected to be low due to the high energy absorption rate

of the tissue. The antenna is suitable for in-body communication at the MedRadio band with an implantable antenna or for off-body communication as a repeater between the implantable antenna and an external far away reader based on the link budget [37]. The square loop is optimized to cover the desired bands using CST software. It has dimensions of 90 mm \times 90 mm with 5.4 mm strip width and 8.6 mm feeding gap.

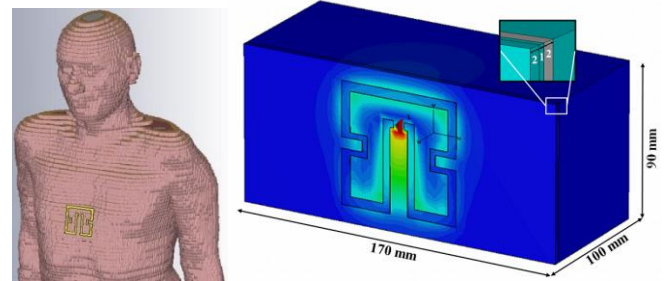


Fig. 4. Gustav voxel body model and a simplified body model that used for the simulation.

The simulated reflection coefficients of the standard square loop and the proposed meandered wearable antenna on the body model are shown in Fig. 5. These antennas have been optimized to match 50 Ω using CST. The proposed loop has a narrower bandwidth due to meandering technique as compared with the conventional loop but still has a sufficient bandwidth of 65 MHz to cover the desired bands.

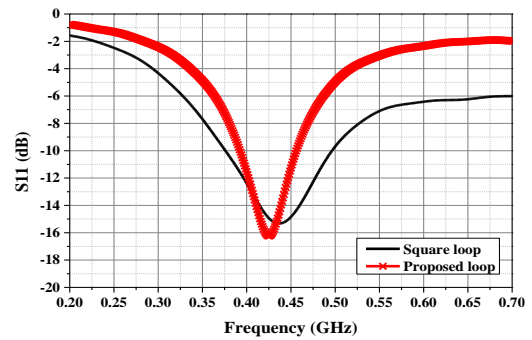


Fig. 5. The simulated reflection coefficients of the proposed meandered loop and the traditional square loop antennas on body model.

B. Magnetic Field Strength

The proposed meandered loop antenna is intended to be attached to the body tissue working as a wearable antenna.

TABLE I
BIO TISSUE BROADBAND PROPERTIES FROM 0.1 – 3 GHz FROM CST VOXEL FAMILY

Prosperities \downarrow Tissue type \rightarrow	Muscle	Fat	Skin
Mue	1	1	1
Rho ρ (kg/m ³)	1041	910	1100
Dielectric constant ϵ_r	57.1	5.6	46.7
Conductivity σ (S/m)	0.79	0.04	0.69
Thermal cond. (W/K/m)	0.53	0.201	0.293

The square loop and the proposed loop antennas were

evaluated using CST Microwave Studio with the Gustav voxel body model and a simplified body model as shown in Fig. 4. The results on both body models are found in good agreement so that the simplified body model was used in most simulations. The size of the simplified body model is chosen to be consistent with the container that is used for measurements as will be shown in Section IV.

The generated magnetic field strength in z-direction for the proposed antenna shown in Fig. 5 was examined along the two major axes of the xy-plane and compared with the conventional square loop antenna as shown in Fig. 6. In this figure, the field of the traditional square loop is shown in grid which is dominant mostly along x axis. The internal area has weak field because the field lines are combined destructively as mentioned before. However, the field still exists although weak because the conductor containing the feeding port has the highest surface current and will contribute higher field. The effect of this weakness on the coupling will be very obvious when the receiver is moved along y-axis. In the case of meandered loop antenna, the combined magnetic fields exist along both x and y axes and stronger than the conventional case as indicated by horizontal bars shown in Fig. 6. It can be noticed that the middle area has the strongest field because it contains the excitation port. The field can be observed in the entire area of the antenna as compared with the traditional one which generates field mostly along the edges. This gives more flexibility and better coupling to the receiver in terms of misalignment in different directions as will be seen in section III.

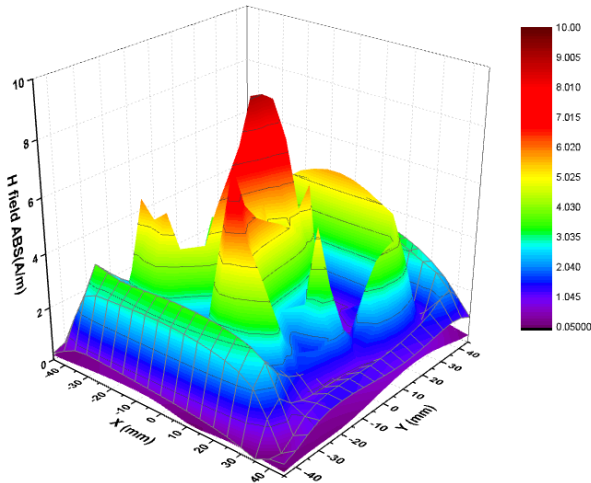


Fig. 6. The magnetic field strength along x and y offsets for the proposed and the square loop antennas. The square loop antenna results are indicated by grids. The results for the proposed meandered loop antenna are indicated by horizontal bars.

C. Specific Absorption Rate

The Specific Absorption Rate (SAR) is an essential factor to measure the absorbed power in the tissue [1], [38]. It is primarily determined by the electric field as shown by

$$SAR = \frac{\sigma|E|^2}{2\rho} \quad (3)$$

where ρ (kg/m^3) is the mass density, σ (S/m) is the conductivity of the tissue and $|E|$ (V/m) is the electric field

intensity.

The maximum transmit power to be used within the safety regulations can be computed according to this value. The FCC SAR regulation of 1.6 W/kg per 1-g averaging was considered to determine the usability of the proposed wearable antenna limits. It is found by calculating the SAR using CST studio that the proposed design can be used with a transmission power of up to 274 mW. This power limit will be considered in evaluation of the antenna performance in terms of WPT.

3. Misalignment Analysis Between Wearable And Implantable Antennas

The misalignment issue breaks the optimum operating condition of the WPT system and the WPT efficiency can be significantly reduced. Because of the magnetic field distribution, the proposed design shows robust performance against the misalignment issue.

To demonstrate the feasibility of the design, an implantable antenna has been optimized based on the same approach as the wearable antenna. This implantable antenna will be used as a receiver to work with the wearable antenna to measure the transmission coefficient S_{21} along different offsets scenarios. The size of the implantable antenna is much smaller than the wearable antenna with a size ratio of 1:18.3.

A. Implantable Antenna

An implantable loop antenna was designed to have a structure similar to the proposed wearable antenna as shown in Fig. 7. The structure was modified from the flat wearable antenna and can be bent around cylindrical implants with minimum dimensions of 11 mm in length and 3.5 mm in radius so that very little space will be occupied by the antenna. This implantable antenna shows broadband response in both cases, flat and bent, as shown in Fig. 8.

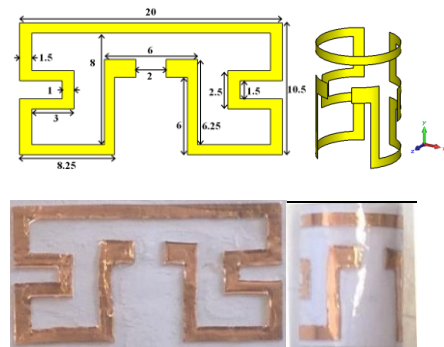


Fig. 7. Dimensions and photographs of the fabricated implantable antenna, all dimensions in mm.

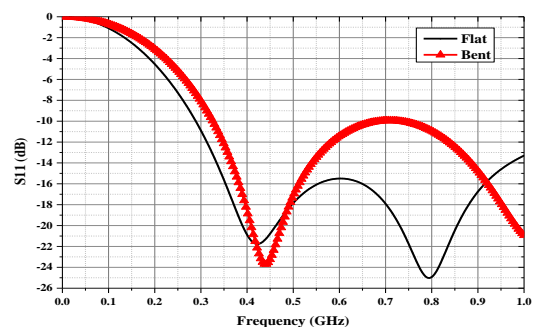


Fig. 8. The reflection coefficient of the proposed implantable antenna in two cases of flat and bent.

Both structures cover well the desired bands of 402-405 MHz and 433 MHz. The radiation efficiency and gain of the implantable antenna are 0.056% and -28.5 dB respectively. These values are expected due to the high loss of body tissues and the small size of the antenna.

The implantable antenna is made of a thin copper sheet with a thickness of 0.04 mm. To prevent direct contact of the antenna material with the tissue, the implantable antenna is surrounded by a thin Polypropylene adhesive tape of 0.04 mm. This thin layer has negligible effect on the antenna performance.

B. Analysis of Misalignment

The misalignment between a pair of wearable and implantable antennas was investigated in terms of S21. The implantable antenna was inserted 30 mm in depth in the body model. It is then shifted along x, y and (x, y) offsets and rotated around the azimuth angle θ as indicated in Fig. 9. The result is compared with a standard square loop pair tested in the same scenario.


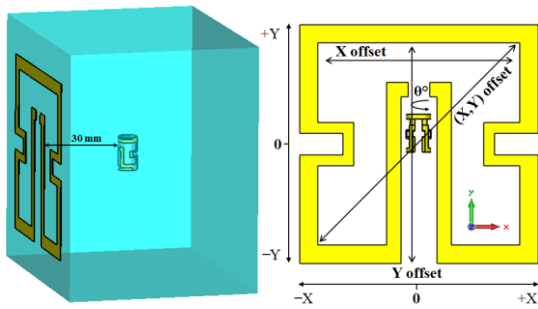



Fig. 9. The setup of testing S₂₁ between the proposed pair of antennas.

The investigation of misalignment is shown in Fig. 10. It is shown that, when the implantable antenna has an offset along the x-axis, the proposed antenna has a similar response to the square loop because of both pairs have relatively strong magnetic fields along the x-axis as shown in Fig. 10(a). But the magnitude of S₂₁ is about 4 dB better as a result of the stronger magnetic field generated by the proposed meandered antenna. Along the y-axis, the effect of the new axis is very obvious. The proposed pair has approximately stable response against offset with a better S₂₁ of 5 dB on average as compared with the square loop as shown in Fig. 10(b). Fig. 10(c) indicates the diagonal offset. The proposed pair has a more stable response compared with the square loop with an advantage of 2 dB up to 7 dB. This advantage comes from the strength of magnetic field along both x and y axes so that the weak coupling from one direction can be compensated by the other direction. The location of the exciting port in the internal area adds more advantages to make the response smoother while the response in the square loop case is more biased toward the side of the exciting port. Another offset was examined by rotating the implantable antenna around the azimuth. The response of both pairs is similar but the proposed design still has a S₂₁ up to 4 dB better as shown in


Fig. 10(d).

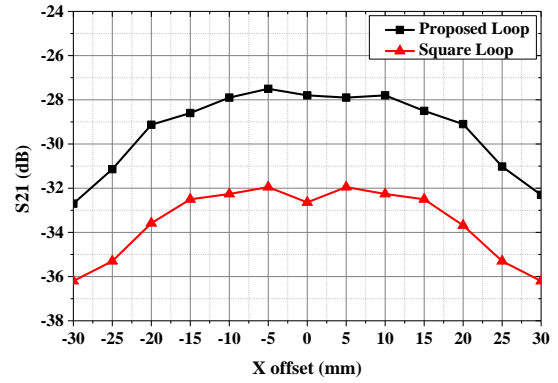


(a)

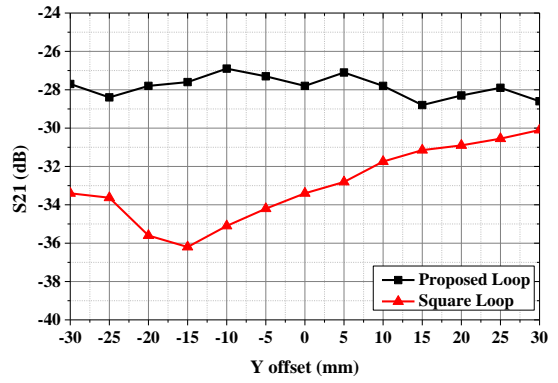

(b)

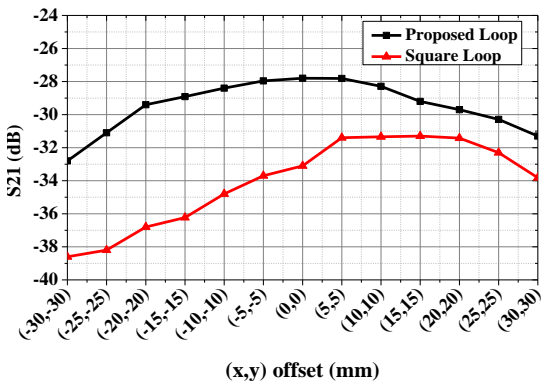

(c)

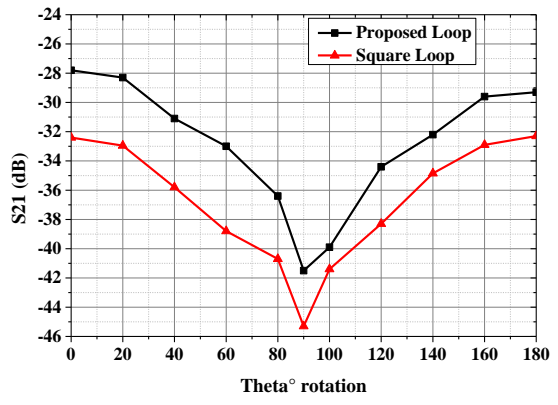

(d)

Fig. 10. The simulated misalignment comparison between the proposed and the square loop antennas along: (a) x-axis, (b) y-axis, (c) (x, y) diagonal and (d) azimuth angle θ .

C. Transmission Coefficient Measurement for the Proposed Design

The proposed wearable and implantable antennas were fabricated and tested in minced pork that mimics human body tissues [9] and [38]. The transmission coefficient S_{21} is measured to evaluate the WPT as shown in Fig. 11.

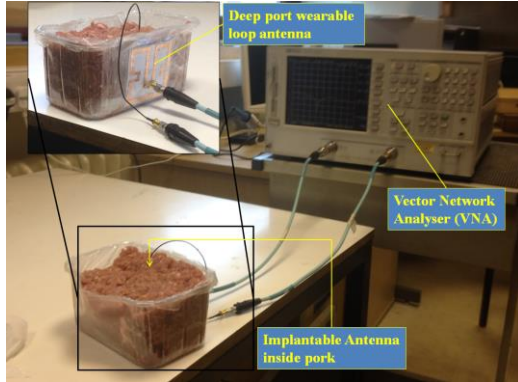


Fig. 11. The comparison of the simulated and measured efficiencies of the rectifier, and measured voltages.

The same procedure of examining S_{21} mentioned in section III B was repeated. The offsets in the x-axis and y-axis directions, diagonally with (x, y) offset, and rotation around the azimuth angle θ were examined. The measured results of S_{21} are in good agreement with the simulated one as depicted in Fig. 12. These results validate the advantage of the

proposed design.

4. Wireless Power Transmission

The WPT is investigated in terms of the real power that can be delivered to the target device using the proposed antennas. A rectifier circuit is developed and integrated with the implantable antenna to form a rectenna. The role of the rectenna is to capture the RF signal from the transmitter and convert it into DC power to be used for powering implantable devices directly or recharging a battery. The design and test of this rectifier will be explained in this section along with the analysis of the maximum power delivery within the safety limits.

A. The Rectifier

A rectifier circuit with a dimension of $10 \text{ mm} \times 5 \text{ mm}$ was designed to be integrated with the implantable antenna. The geometry detail of the rectifier with component values is shown in Fig. 13. This design is based on the principle of voltage doubler circuit using dual zero bias Schottky diodes HSMS-2822 from AVAGO Technologies [39]. The Advanced Design System software 2011.01 was used to develop the circuit. The optimization process to miniaturize this rectifier is based on reducing the size of transmission lines and then the overall performance of the rectifier can be compensated by tuning the values of the lumped elements. The lumped components are approximated then to realistic values and the size of the transmission lines is slightly changed to retrieve the optimum performance of the rectifier.

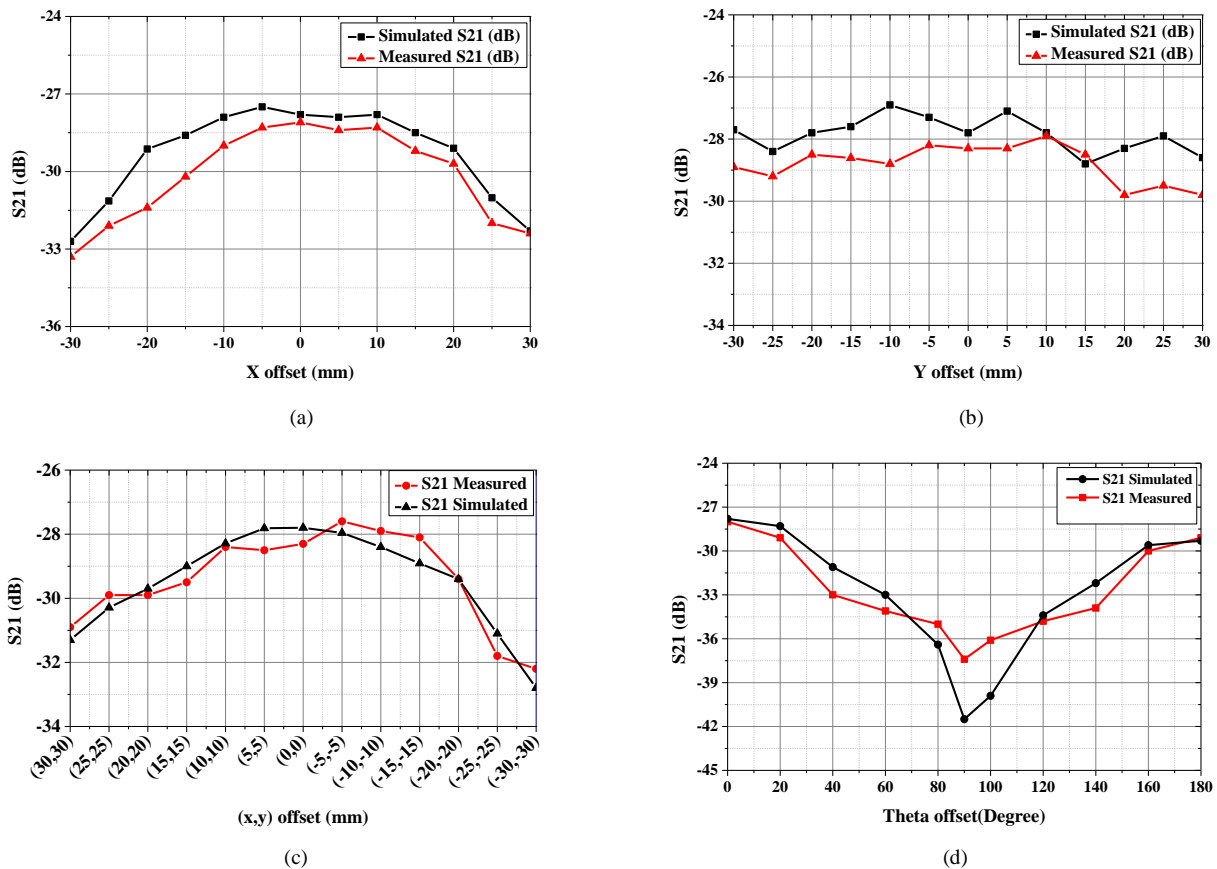


Fig. 12. The simulated and measured transmission coefficients of the proposed pair antennas with offsets along: (a) x-axis, (b) y-axis, (c) (x, y) diagonal (x,y) and (d) Theta offset

This process is repeated many times to get smaller rectifier until reach the maximum miniaturization. An LC matching circuit is used to convert the input impedance of the rectifier to 50Ω so that it can be connected directly to the antenna.

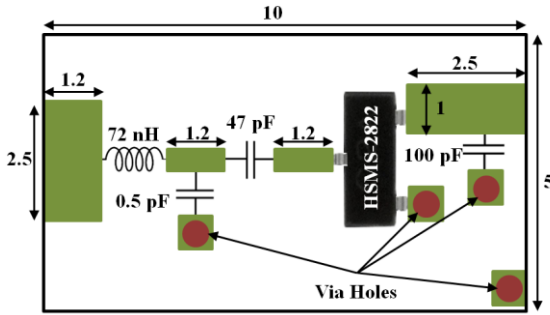


Fig. 13. The geometry of the designed rectifier, all dimensions in mm.

The rectifier showed the best response on a load value of $4.7 K\Omega$. It has an RF to DC conversion efficiencies of 28% at -10 dBm input power up to more than 70% at 10 dBm input power. This rectifier can offer more than 50% efficiency when the input power is larger than -4 dBm. The main reason for the difference in efficiency is because the impedance of the diode changes with the input power level and hence the efficiency of the rectifier is a function of the input power. The circuit was fabricated on a Duroid 5880 substrate with a relative dielectric constant of 2.2 and a thickness of 1.57 mm.

The measurement setup is shown in Fig. 14. It consists of a signal generator to feed the rectifier and a multimeter to measure the voltage on the load. A range of input powers at 433 MHz have been applied to the circuit. It showed a 50% rectification efficiency with input power -4 dBm and the efficiency was increasing with the rising the input power level until the value 10 dBm where the efficiency is saturated at around 76%. The simulated and measured efficiencies are in very good agreement as depicted in Fig. 15.

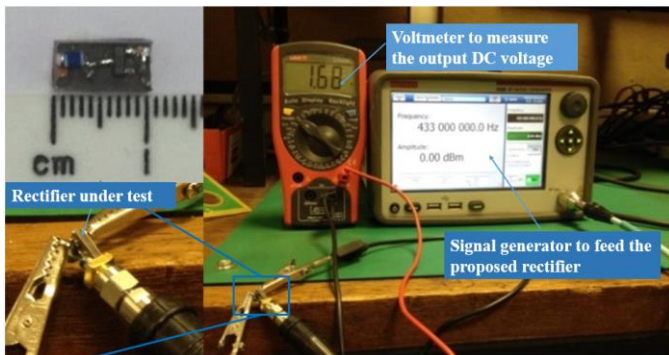


Fig. 14. The measurement setup of the proposed rectifier.

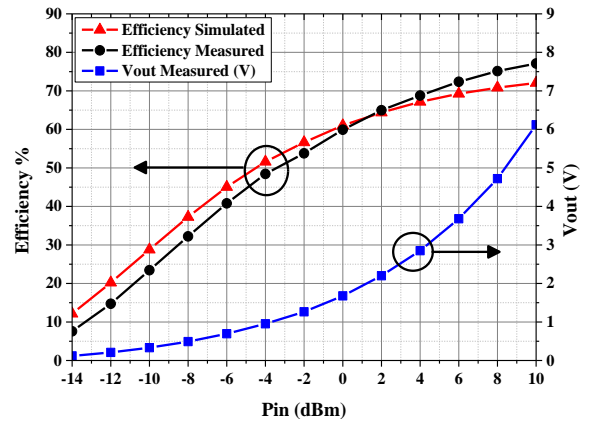


Fig. 15. The comparison of the simulated and measured efficiencies of the rectifier, and measured voltages.


B. Maximum Power Delivery

limit is tested using the wearable antenna and implantable rectenna. First, the proposed design was tested under low input power of 10 mW to demonstrate the ability of the system in delivering sufficient power to the load. The experiment setup contains a signal generator, a cubic container with dimensions $9 \text{ cm} \times 10 \text{ cm} \times 17 \text{ cm}$ filled with minced pork to mimic body tissue and a voltmeter to measure the voltage as shown in Fig. 16(a). A 50Ω coaxial cable is used to connect the implantable antenna to the rectifier. It is worth mentioning that the coaxial cable has no effect on the coupling strength where a bead had been added on the connector. The measurement was not significantly changed by these efforts. With 10 mW input power available to the wearable antenna, the received power at the load was $13 \mu\text{W}$.


A power amplifier was used to boost the level of the transmit power up to 274 mW as shown in Fig. 16(b). Both the output DC voltage and the power are measured against a range of input power not exceeding the safety limit according to the SAR as shown in Fig. 17. The total power transfer efficiency is defined by

$$\eta = \frac{P_{dc}}{P_{in}} \times 100 \quad (4)$$

where η is the total wireless power transfer efficiency including RF to RF and RF to DC conversion efficiencies. P_{dc} and P_{in} are the power delivered to the load and the power available to the transmitting wearable antenna respectively.

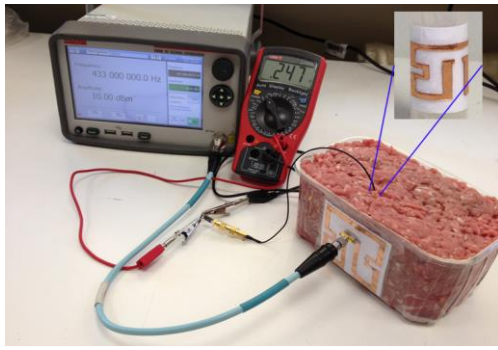

(a)

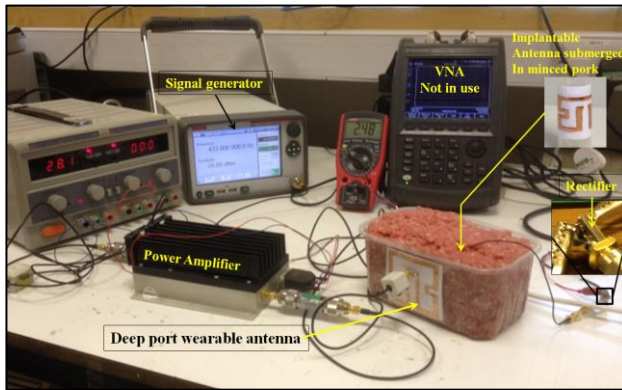

(b)

Fig. 16. The experiment setup of measuring the output power versus different input power: (a) with a constant input power of 10 dBm (b) with a sweep of input power.

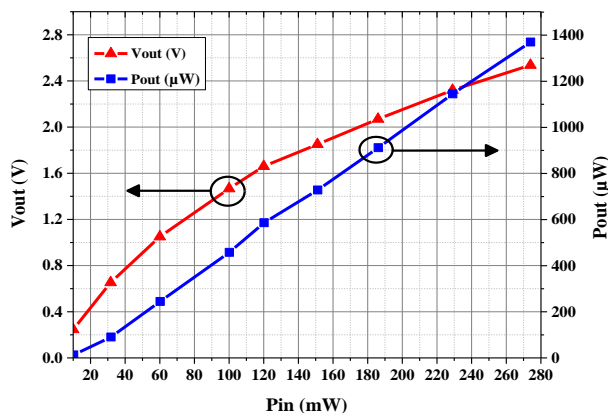


Fig. 17. The measured output power and voltage as a function of the input power.

These results indicate a total power transfer efficiency of 0.1 % when the power available to the wearable antenna is 10 mW. The efficiency is relatively low mainly because of the low RF to RF transfer efficiency due to the high tissue loss. The efficiency can be increased up to 0.5 % when the available power exceeded 50 mW.

A DC power of more than 1000 μW can be harvested with an input power under safety limits. The received power is enough to power many common implantable medical devices such as a pacemaker, a nerve stimulation device and a glucose measurement system that requires 70 μW [40], 100 μW [41] and 48 μW [42] power, respectively.

5. Conclusion

This paper presents a novel approach to design a meandered loop antenna that generates strong magnetic fields along two orthogonal axes. The new design shows significant advantages in terms of improving WPT and the robustness to the misalignment issue.

Two meandered loop antennas are designed based on the same approach to form a pair of compatible wearable and implantable antennas. The proposed pair was compared with a pair of conventional square loop antennas. The new design showed very good tolerance against the misalignment in different directions and better power transmission. Then a rectifier circuit of the size of 10 mm \times 5 mm was designed and optimized to be used with the implantable antenna to form a rectenna. The rectenna works with the wearable antenna as a WPT system. This rectifier performs RF to DC conversion with an efficiency of 50% to 70% at the input power from -4 dBm to 10 dBm.

The measured results validated the simulated one. The overall results demonstrated the significant advantages of the proposed design. The output DC voltage and power with respect to different inputs within the safety limits were measured. A DC power of more than 1000 μW can be harvested under the condition that the transmitted power by the wearable antenna is under safety limits. This amount of power is more than enough to directly power many common implantable medical devices including the pacemaker, the nerve stimulation device and the glucose measurement system.

REFERENCES

- [1] J. M. Rabaey, M. Mark, D. Chen, C. Sutardja, C. Tang, S. Gowada, M. Wagner and D. Werthimer, "Powering and Communicating with mm-Size Implants," *Design, Automation & Test in Europe Conference & Exhibition (DATE)*, 2011.
- [2] J. S. Ho, K. Sanghoek, and A. S. Y. Poon, "Midfield Wireless Powering for Implantable Systems," *Proceedings of the IEEE*, vol. 101, pp. 1369-1378, 2013.
- [3] C. Liu; Y. Guo; H. Sun; S. Xiao, "Design and Safety Considerations of an Implantable Rectenna for Far-Field Wireless Power Transfer," *IEEE Transactions on Antennas and Propagation*, vol.62, no.11, pp.5798-5806, Nov. 2014.
- [4] S. Bakogianni and S. Koulouridis, "A Dual-Band Implantable Rectenna for Wireless Data and Power Support at Sub-GHz Region," in *IEEE Transactions on Antennas and Propagation*, vol. 67, no. 11, pp. 6800-6810, Nov. 2019.
- [5] H. Lyu, P. Gad, H. Zhong, V. R. Edgerton and A. Babakhani, "A 430-MHz Wirelessly Powered Implantable Pulse Generator With Intensity/Rate Control and Sub-1 μA Quiescent Current Consumption," in *IEEE Transactions on Biomedical Circuits and Systems*, vol. 13, no. 1, pp. 180-190, Feb. 2019.
- [6] M. Kod et al., "Feasibility Study of Using the Housing Cases of Implantable Devices as Antennas," in *IEEE Access*, vol. 4, pp. 6939-6949, 2016.
- [7] H. Zhang, S. Gao, T. Ngo, W. Wu and Y. Guo, "Wireless Power Transfer Antenna Alignment Using Intermodulation for Two-Tone Powered Implantable Medical Devices," in *IEEE Transactions on Microwave Theory and Techniques*, vol. 67, no. 5, pp. 1708-1716, May 2019.
- [8] M.K. Hosain, A.Z. Kouzani, S.J. Tye, O.A. Abulseoud, A. Amiet, A. Galehdar, A. Kaynak, M. Berk, "Development of a Compact Rectenna for Wireless Powering of a Head-Mountable Deep Brain Stimulation Device," *IEEE Journal of Translational Engineering in Health and Medicine*, vol.2, no., pp.1-13, 2014
- [9] F. Huang; C. Lee; C. Chang; L. Chen; T. Yo; C. Luo, "Rectenna Application of Miniaturized Implantable Antenna Design for Triple-

- Band Biotelemetry Communication," *IEEE Transactions on Antennas and Propagation*, vol.59, no.7, pp.2646-2653, July 2011.
- [10] T. Campi, S. Cruciani, F. Palandrani, V. De Santis, A. Hirata and M. Feliziani, "Wireless Power Transfer Charging System for AIMDs and Pacemakers," *IEEE Transactions on Microwave Theory and Techniques*, vol. 64, no. 2, pp. 633-642, Feb. 2016.
- [11] M. Machnoor, E. S. Gámez Rodríguez, P. Kosta, J. Stang and G. Lazzi, "Analysis and Design of a 3-Coil Wireless Power Transmission System for Biomedical Applications," in *IEEE Transactions on Antennas and Propagation*, vol. 67, no. 8, pp. 5012-5024, Aug. 2019.
- [12] E. Y. Chow, C. L. Yang, A. Chlebowski, S. Moon, W. J. Chappell and P. P. Irazoqui, "Implantable Wireless Telemetry Boards for In Vivo Transocular Transmission," *IEEE Transactions on Microwave Theory and Techniques*, vol. 56, no. 12, pp. 3200-3208, Dec. 2008.
- [13] G. Sun, B. Muneer, Y. Li and Q. Zhu, "Ultracompact Implantable Design With Integrated Wireless Power Transfer and RF Transmission Capabilities," in *IEEE Transactions on Biomedical Circuits and Systems*, vol. 12, no. 2, pp. 281-291, April 2018.
- [14] J. Kim, D. H. Kim, J. Choi, K. H. Kim and Y. J. Park, "Free-Positioning Wireless Charging System for Small Electronic Devices Using a Bowl-Shaped Transmitting Coil," *IEEE Transactions on Microwave Theory and Techniques*, vol. 63, no. 3, pp. 791-800, March 2015.
- [15] M. Q. Nguyen, Z. Hughes, P. Woods, Y. S. Seo, S. Rao and J. C. Chiao, "Field Distribution Models of Spiral Coil for Misalignment Analysis in Wireless Power Transfer Systems," *IEEE Transactions on Microwave Theory and Techniques*, vol. 62, no. 4, pp. 920-930, April 2014.
- [16] A.N. Laskovski, M.R. Yuce, T. Dissanayake, "Stacked Spirals for Biosensor Telemetry," *IEEE in Sensors Journal*, vol.11, no.6, pp.1484-1490, June 2011.
- [17] A.D. Rush, P.R. Troyk, "A Power and Data Link for a Wireless-Implanted Neural Recording System," *IEEE Transactions on Biomedical Engineering*, vol.59, no.11, pp.3255-3262, Nov. 2012.
- [18] K.M. Silay, C. Dehollain, M. Declercq, "A Closed-Loop Remote Powering Link for Wireless Cortical Implants," *IEEE Sensors Journal*, vol.13, no.9, pp.3226-3235, Sept. 2013.
- [19] G. Monti, P. Arcuti and L. Tarricone, "Resonant Inductive Link for Remote Powering of Pacemakers," *IEEE Transactions on Microwave Theory and Techniques*, vol. 63, no. 11, pp. 3814-3822, Nov. 2015.
- [20] Z. N. Chen, G. C. Liu, and T. S. P. See, "Transmission of RF Signals Between MICS Loop Antennas in Free Space and Implanted in the Human Head," *IEEE Transactions on Antennas and Propagation*, vol.57, no.6, pp.1850-1854, June 2009.
- [21] A. Kiourti, J.R. Costa, C.A. Fernandes, K.S. Nikita, "A Broadband Implantable and a Dual-Band On-Body Repeater Antenna: Design and Transmission Performance," *IEEE Transactions on Antennas and Propagation*, vol.62, no.6, pp.2899-2908, June 2014.
- [22] M. Manoufali, K. Bialkowski, B. J. Mohammed, P. C. Mills and A. Abbosh, "Near-Field Inductive-Coupling Link to Power a Three-Dimensional Millimeter-Size Antenna for Brain Implantable Medical Devices," in *IEEE Transactions on Biomedical Engineering*, vol. 65, no. 1, pp. 4-14, Jan. 2018.
- [23] T. Shaw and D. Mitra, "Metasurface-based radiative near-field wireless power transfer system for implantable medical devices," in *IET Microwaves, Antennas & Propagation*, vol. 13, no. 12, pp. 1974-1982, 2 10 2019.
- [24] M. Kod, J. Zhou, Y. Huang, R. Alrawashdeh and M. Hussein, "Dual Broadband Butterfly Loop Antenna for In-Body Wearable Applications," *Antennas and Propagation Conference (LAPC)*, Loughborough, 2015.
- [25] S. O'Driscoll, A.S.Y. Poon, T.H. Meng, "A mm-sized implantable power receiver with adaptive link compensation," *IEEE International Conference on Solid-State Circuits*, vol., no., pp.294-295,295a, 8-12 Feb. 2009.
- [26] Z. Chen, H. Sun and W. Geyi, "Maximum Wireless Power Transfer to the Implantable Device in the Radiative Near Field," in *IEEE Antennas and Wireless Propagation Letters*, vol. 16, pp. 1780-1783, 2017.
- [27] R. Das and H. Yoo, "A Multiband Antenna Associating Wireless Monitoring and Nonleaky Wireless Power Transfer System for Biomedical Implants," in *IEEE Transactions on Microwave Theory and Techniques*, vol. 65, no. 7, pp. 2485-2495, July 2017.
- [28] S. Amendola, E. Moradi, K. Koski, T. Bjorninen, L. Sydanheimo, L. Ukkonen, J.M. Rabaey, Y. Rahmat-Samii, "Design and optimization of mm-size implantable and wearable on-body antennas for biomedical systems," *Antennas and Propagation (EuCAP)*, 2014.
- [29] A. K. RamRakhyani and G. Lazzi, "Multicoil Telemetry System for Compensation of Coil Misalignment Effects in Implantable Systems," *IEEE Antennas and Wireless Propagation Letters*, vol. 11, no. , pp. 1675-1678, 2012.
- [30] M. Q. Nguyen, Y. Chou, D. Plesa, S. Rao and J. C. Chiao, "Multiple-Inputs and Multiple-Outputs Wireless Power Combining and Delivering Systems," *IEEE Transactions on Power Electronics*, vol. 30, no. 11, pp. 6254-6263, Nov. 2015.
- [31] S. G. Lee, H. Hoang, Y. H. Choi and F. Bien, "Efficiency improvement for magnetic resonance based wireless power transfer with axial-misalignment," *Electronics Letters*, vol. 48, no. 6, pp. 339-340, March 15 2012.
- [32] Z. Zhang and K. T. Chau, "Homogeneous Wireless Power Transfer for Move-and-Charge," *IEEE Transactions on Power Electronics*, vol. 30, no. 11, pp. 6213-6220, Nov. 2015.
- [33] J. P. W. Chow, N. Chen, H. S. H. Chung and L. L. H. Chan, "An Investigation Into the Use of Orthogonal Winding in Loosely Coupled Link for Improving Power Transfer Efficiency Under Coil Misalignment," *IEEE Transactions on Power Electronics*, vol. 30, no. 10, pp. 5632-5649, Oct. 2015.
- [34] J. Kim, D. H. Kim, J. Choi, K. H. Kim and Y. J. Park, "Free-Positioning Wireless Charging System for Small Electronic Devices Using a Bowl-Shaped Transmitting Coil," *IEEE Transactions on Microwave Theory and Techniques*, vol. 63, no. 3, pp. 791-800, March 2015.
- [35] W.-S. Lee, S. Park and J. Lee, "A loosely coupled distributed antenna array for lateral misalignment-improved near-field wireless power transfer system," *Microwave and Optical Technology Letters*, vol. 57, issue 12, pp. 2829-2833, December 2015.
- [36] R. Alrawashdeh, Y. Huang, and P. Cao, "Flexible meandered loop antenna for implants in MedRadio and ISM bands," *Electronics Letters*, vol. 49, pp. 1515-1516, Nov 21 2013
- [37] S. Agneessens, P. V. Torre, E. Tanghe, G. Vermeeren, W. Joseph, and H. Rogier, "On-Body Wearable Repeater as a Data Link Relay for In-Body Wireless Implants," *IEEE Antennas and Wireless Propagat. Letters*, vol. 11, pp. 1714 - 1717, 2012.
- [38] R. Alrawashdeh, Y. Hunag, M. Kod, A. A. B. Sajak, "A Broadband Flexible Implantable Loop Antenna with Complementary Split Ring Resonators," *IEEE Antennas and Wireless Propagation. Letters*, 2015.
- [39] Surface Mount RF Schottky Barrier Diodes, Data Sheet. Avago Technologies, November 26, 2014.
- [40] R. Das, H. Yoo, "Biotelemetry and Wireless Powering for Leadless Pacemaker Systems," *IEEE in Microwave and Wireless Components Letters*, vol.25, no.4, pp.262-264, April 2015.
- [41] C. Niu; H. Hao; L. Li; B. Ma; M. Wu, "The Transcutaneous Charger for Implanted Nerve Stimulation Device," *28th Annual International Conference of the IEEE in Engineering in Medicine and Biology Society. EMBS '06.*, vol., no., pp.4941-4944, 2006.
- [42] K. Bazaka, M.V. Jacob, "Implantable Devices: Issues and Challenges", *Electronics*. 2(1):1-34, 2013.